

DASH APEX

6, 12, and 24









Operator's Manual



TABLE OF CONTENTS

Symbols.....	1
Caution Warning Statements	2
Model Description	4
Features	4
Intended Use	4
Warranty.....	4
How To Video Links	5
Initial Setup.....	5
Quick Start	6
Settings	7
Operation.....	8
Review Cycle Time and Speed Settings.....	8
Changing Cycle Time and Speed Settings	8
Balancing Loads	9
Care and Preventative Maintenance	10
Cleaning and Disinfection	10
Troubleshooting	11
General Specifications	13
Calculating the G-Force	16
Replacement Parts.....	17
Dash Apex 6	17
Dash Apex 12	17
Dash Apex 24	18
Previous Manual Revisions	18

SYMBOLS

Symbol	Definition	Use
	Caution	Caution to safety hazard. Potential risk of personal injury or damage to the instrument if improperly handled. Consult the manual before proceeding.
	Manufacturer	Manufacturer of record.
	Electrical and electronic products recycling symbol	Recycle only as electronic waste. Do not dispose in normal waste.
	RoHS Compliant	Compliance with RoHS environmental standards.
	CE Mark	Denotes conformity to specific European directives and regulations.
	MET Listing	Denotes conformity to specific safety standards and regulations.
	UK Mark	Denotes conformity to specific UK directives and regulations.
FDA LISTED	FDA Listed	Denotes that the product has been properly listed with the FDA.
	ISO Certification	Denotes conformity to quality standards and quality management systems.

CAUTION WARNING STATEMENTS



This device is intended to be operated by properly trained personnel who have carefully read the operating manual and are familiar with the function of the device. Users should also comply with the specimen receptacle manufacturer's specific instructions for use, in addition to any other protocols established by the testing organization.



WARNING: For the safety of both the operator and service personnel, care should be taken when using this centrifuge if handling substances that are known to be toxic, radioactive or contaminated with pathogenic microorganisms. Use appropriate personal protection equipment (PPE). When Risk Group II materials are used, (as identified in the World Health Organization "Laboratory Bio-Safety Manual"), a Bio- Seal should be employed. In the event that materials of a higher risk group are being used, more than one level of protection must be provided. The use of flammable or explosive materials as well as those materials which have a vigorous chemical reaction is prohibited.



Unplug the centrifuge before cleaning or performing maintenance.



WARNING: Inspect centrifuge for cracks or physical damage to cabinet, lid, rotor, or tube holders. Damage may result in unsafe operation. Discontinue use until repairs have been performed.



The use of flammable or explosive materials as well as those materials which have a vigorous chemical reaction is prohibited.



For your safety and durability of the machine, never transport or store centrifuge with tube holders inside the machine.



WARNING: "Universal precautions"¹ should be followed in handling all items contaminated with blood or other bodily fluids.



This equipment generates, uses, and can radiate radio frequency energy, and if not installed and used in accordance with this operator manual, may cause interference to radio communications.



Operation of this equipment in a residential area may cause interference, in which case the user will be required to correct the interference at his own expense.



Operation of this equipment in a manner not specified by the manufacturer may impair the protection provided by the equipment.



Electrical Safety protection is provided by properly connecting the centrifuge to earth ground. Use only the manufacturer provided line cord and ensure that it is connected to a properly grounded power receptacle. Failure to do so will result in an electrical hazard.



WARNING: Do not make modifications to or remove any hardware from rotor without prior authorization from Drucker Diagnostics.



WARNING: Only use Drucker Diagnostics components in this centrifuge.



Due to the lack of the possibility of human exposure, all Drucker centrifuges and accessories sold by Drucker Diagnostics, Inc. are compliant without any special labeling required by the California Safe Drinking Water and Toxic Enforcement Act (Proposition 65).

1 Recommendations for Prevention of HIV Transmission in Health Care Settings. MMWR 1987; 36 (Supplement #2S)

MODEL DESCRIPTION

DASH Apex is engineered for STAT sample processing. When used with the Drucker DASH Approach to centrifugation, the DASH Apex cuts your turnaround time (TAT) by up to 20 minutes.

This general-purpose laboratory centrifuge may also be used to spin approved containers with biologics, chemicals (non-flammable, non-explosive, non-volatile, and non-highly reactive), and environmental samples.

FEATURES

- Simple 2-Button interface
- Three (3) easily selectable pre-set cycles are conveniently labeled for your lab's most common applications. Use the default cycles or settings can be customized. An LED light indicates the current selected setting.
- If desired, the control panel can be locked on one preset cycle, ideal for standardization to a single spin.
- Lid lighting indicates the centrifuge's status (ready, running, done), keeping your TAT down (patent pending).
- A traditional audible alert indicates the completion of the cycle.
- Cool-Flow air flow design prevents overheating of samples by maintaining room temperature.
- Carbon fibers are used to reinforce the tube holders and provide high strength and durability.
- A clear lid permits safe observation of samples and optical calibration of speed.
- The lid safety system only allows entry into the centrifuge after the rotor has completely stopped.
- The lid safety system prevents the centrifuge from operating unless the lid is closed and latched.
- The high-power brushless DC motor provides years of operation with no routine maintenance.

INTENDED USE

General purpose laboratory centrifuge, intended for the density-based separation of fluids through centripetal acceleration.

WARRANTY

Drucker Diagnostics warrants that this centrifuge is free from defects in workmanship and parts for 2 years.

HOW TO VIDEO LINKS

To access our How To Video, please click the relevant link below:

[Dash Apex 12](#)


INITIAL SETUP

- Unpack and verify that all the following are included:
 - Centrifuge
 - Power cord
 - Tube holders: 6 for Apex 6, 12 for Apex 12, or 6 buckets for Apex 24
 - Quick Start Guide
- Setup the centrifuge on flat and level surface. A bench top clearance height of 21" (54 cm) is required to open the lid.
- The centrifuge should have 6" (15 cm) of clear space around the centrifuge. Proper ventilation is necessary to prevent the overheating of samples as well as premature failure of the centrifuge. Choose an area which allows unencumbered air flow, and where the temperature remains between 16°C and 32°C.
- No hazardous material shall be permitted in the clearance envelope during operation.
- The operator time within the envelope shall be limited to the time necessary for loading, unloading, and centrifuge operation only.
- Plug the line cord into the centrifuge.
- Plug the line cord into an electrical outlet.
- Turn on the power switch on the back of the centrifuge




Be sure the electrical outlet is always accessible as the line cord is the means of emergency Disconnection!


DASH Apex 6

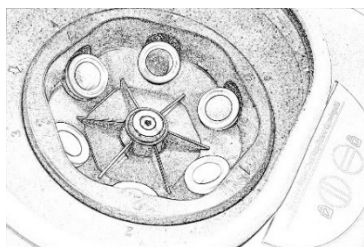

DASH Apex 12

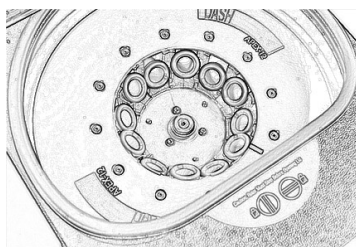


DASH Apex 24

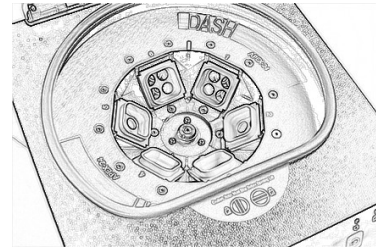

QUICK START

The LED indicator light is on for the cycle currently selected. Depending on your unit, you may have the following cycles:


Barricor™:	For BD Vacutainer® Barricor™ tubes
Coag:	For Coagulation or Platelet Poor Plasma (PPP)
PST/SST™:	For BD PST™ & SST™ tubes with gel or blood tubes without gel
Chemistry:	For BD PST™ II & SST™ II tubes with gel or blood tubes without gel
3 Min:	STAT centrifugation at 4,000 xg
5 Min:	STAT centrifugation at 4,000 xg (6 and 12) or 3,000 xg (24)
6 Min:	STAT centrifugation at 3,000 xg
Custom:	This setting can be customized to your lab's validated cycles.

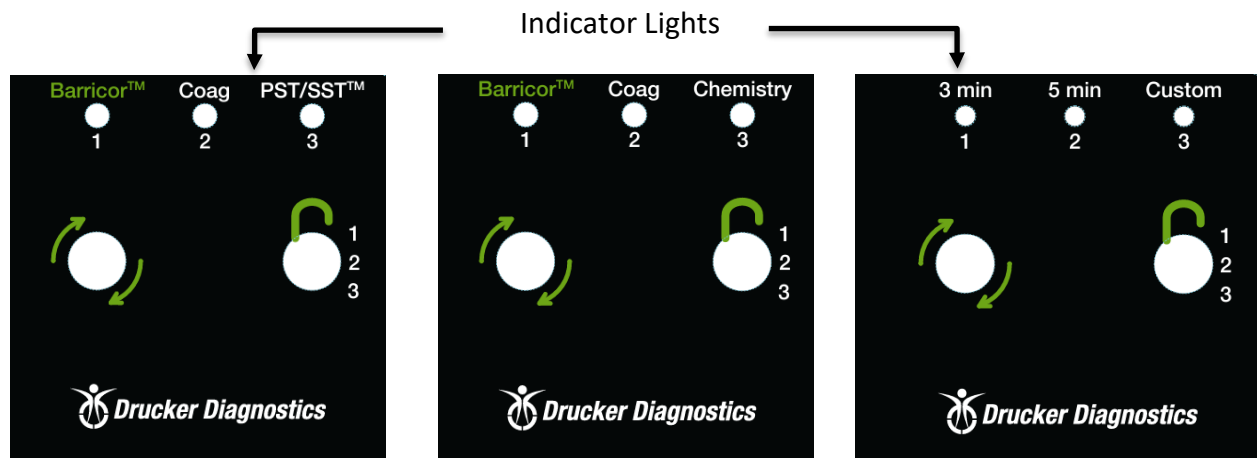

	Start	Begins running the cycle indicated by the cycle indicator LED light. The lid must be closed.
	Unlock	Allows access into the rotor chamber by disengaging the locking mechanism. Entry is only possible when the rotor is stopped.
	Stop	Pressing the UNLOCK button during operation will terminate the run and unlock the lid after the rotor has come to a stop.

	Cycle Selection	The LED light above the numbers indicates the cycle currently selected. To change the selected cycle, open the lid and press the UNLOCK button in succession until the desired cycle is selected. Two seconds after selection, the button reverts to its UNLOCK function.
	Lock Cycle Selection	Open lid. Select desired cycle. Press and hold the UNLOCK button for 5 seconds. Two beeps will confirm that cycle selection is locked.
	Unlock Cycle Selection	To re-enable cycle selection, open lid, then press and hold the UNLOCK button for 5 seconds. Three beeps will confirm that cycle selection is now unlocked.

SETTINGS



Factory Settings	DASH Apex 6			DASH Apex 12			DASH Apex 24		
Cycle	RPM	Time	G-Force	RPM	Time	G-Force	RPM	Time	G-Force
3 min	5,300	3	4,000	5,200	3	4,000	4,200	5	3,000
5 min	5,300	5	4,000	5,200	5	4,000	4,200	6	3,000
Custom	3,800	7	2,000	3,600	7	2,000	3,500	7	2,000



Factory Settings	DASH Apex 6			DASH Apex 12			DASH Apex 24		
Cycle	RPM	Time	G-Force	RPM	Time	G-Force	RPM	Time	G-Force
Barricor™	5,300	3	4,000	5,200	3	4,000	4,200	5	3,000
Coag	5,300	5	4,000	5,200	5	4,000	4,200	6	3,000
PST/SST™	3,800	7	2,000	3,600	7	2,000	3,500	7	2,000



Factory Settings	DASH Apex 6			DASH Apex 12			DASH Apex 24		
Cycle	RPM	Time	G-Force	RPM	Time	G-Force	RPM	Time	G-Force
Barricor™	5,300	3	4,000	5,200	3	4,000	4,200	5	3,000
Coag	5,300	5	4,000	5,200	5	4,000	4,200	6	3,000
Chemistry (PSTII/SSTII™)	4,600	5	3,000	4,400	5	3,000	4,300	5	3,000

Cycle	Tube Type	RPM	G-Force (RCF)
1			
2			
3			

Custom cycles, if desired:

NOTE: Timer starts when speed reaches 90% of set speed. Deceleration time is not included in cycle time.

OPERATION

- Place the tubes into the tube holders. Be sure to follow the rules for balanced loads as listed on page 9.
- The front panel LED is illuminated for the currently selected cycle. The selected cycle determines the run time and speed. To select another cycle, press the UNLOCK button in succession until the desired cycle is selected. Note: cycle selection is only available with the lid open.
- Close the lid and turn the lid knob clockwise to its complete stop position.
- Pushing the START button on the control panel starts the spin cycle.
- When the cycle is completed, the rotor will slow to a complete stop and the lid light will flash.
- The locking mechanism will disengage for 60 seconds allowing entry into the rotor chamber. To unlock after more than 60 seconds have elapsed, press the UNLOCK button. The lid will unlock for another 15 seconds.
- Turn the lid knob counterclockwise and open the lid. The lid light will turn off.
- You may now safely remove the samples.

REVIEW CYCLE TIME AND SPEED SETTINGS

Your settings may not be standard. To review current settings, follow this procedure:

- Open the lid. The lid must be opened to review the selected cycle time and speed.
- Press and hold the START button until you hear a beep.
- Release the START button, the centrifuge will beep and the LED light will flash once for each minute of run time in the current cycle. 10 beeps / flashes equal 10 minutes of run time.
- Pressing the START button again will cause the unit to beep and the LED light to flash once for each 100 revolution per minute (RPM) in the current cycle. 10 beeps / flashes equal 10 x 100 or 1,000 RPM.
- The centrifuge will automatically revert to normal mode at the end.

CHANGING CYCLE TIME AND SPEED SETTINGS

- Open the lid. The lid must be opened to change the selected cycle time and speed.
- Select the cycle you wish to change.
- Press and hold the START and UNLOCK buttons together until the LED light flashes.
- Press the START button for each minute of run time.
- Move to speed setting mode by pressing the UNLOCK button.
- Press the START button once for each 100 rpm.
- Press the UNLOCK button to exit setting mode.


BALANCING LOADS




Your centrifuge must contain a balanced load to work properly. Spinning balanced loads will extend the life of the centrifuge and produce better results. Use the following rules when loading the rotor. If an odd number of samples is to be spun, fill a tube with water to match the weight of the unpaired sample and place it across from this sample.

*Opposing tube holders must be equally loaded or empty or loaded with equally weighted samples.
When loading only 3 tubes, they must be of equal weight.*

6 Tube Centrifuges

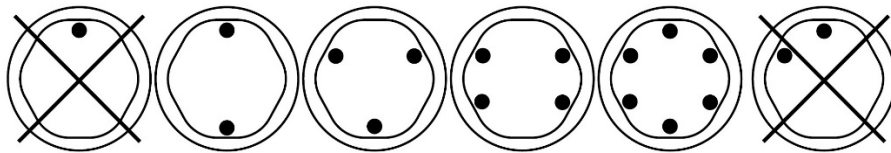


12 Tube Centrifuges

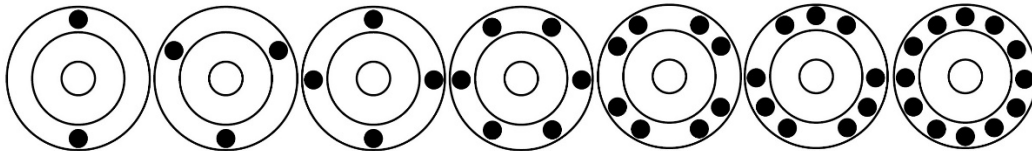


24 Tube Centrifuges

Balanced Rotor Loading

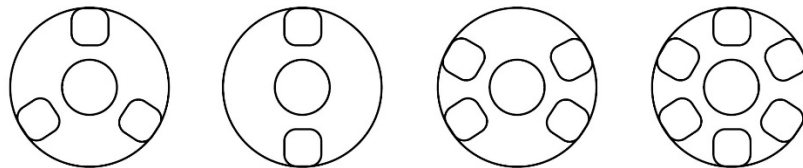

Proper Bucket Loading

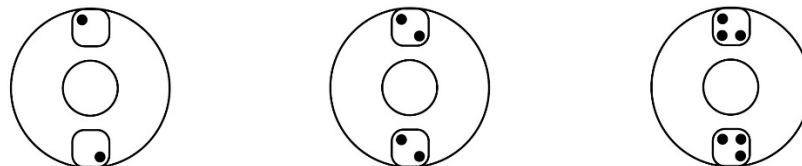

*Buckets can be placed around the rotor in any of the rotor loading configurations shown.
Each bucket must be loaded symmetrically with tubes as above.*

CARE AND PREVENTATIVE MAINTENANCE

With proper care and maintenance, your centrifuge will provide years of laboratory service. For proper care, the following steps should be taken:

- **Always Spin Balanced Loads:** Make certain that you are always spinning a balanced load, as shown in the previous section. These centrifuges have a unique counter balanced motor mounting design which produces excellent vibration dampening. However, out-of-balance loads may break glass test tubes and may produce unsatisfactory separation results. Proper load balancing will improve sample separation and extend the life of the centrifuge.
- **Motor and Electrical Maintenance:** The highest quality electrical components have been selected for the DASH Apex centrifuges and should not need maintenance or servicing for the life of the centrifuge.
- **Tube Holder Replacement:** It is recommended that the tube holders be replaced after 24 months of use. Inspect tube holders regularly for cracks. If cracks are discovered, replace immediately.
- **Remove Accessories Before Moving:** All tube holders, samples, and caps must be removed from the rotor chamber before transporting or storing the centrifuge to prevent damage and injury.

CLEANING AND DISINFECTION

To prolong the life of the centrifuge, cleaning and disinfection is recommended every six months or whenever there is a spillage or tube breakage. Contaminants must be removed immediately or corrosion and premature degradation of components can occur. Before using any cleaning or decontamination methods other than those recommended by the manufacturer, users should verify with the manufacturer that the proposed method will not damage the equipment.



Cleaning and Decontamination may be necessary as a safeguard before laboratory centrifuges, rotors, and any accessories are maintained, repaired, or transferred.

- Unplug the centrifuge before cleaning.
- Use appropriate personal protective equipment (PPE).
- Apply Cleaning solutions with a dampened towel or cloth ONLY. Do not spray or pour cleaning solution directly onto or into the centrifuge. Do not saturate or submerge the centrifuge in water or other cleaning solutions as this will cause damage, create a safety risk, and void the warranty.
- ONLY isopropyl alcohol or a 10% (5500 PPM) bleach solution should be used to disinfect the centrifuge and its accessories.
- All surfaces must be dried immediately after cleaning and disinfecting.



TBQ GERMICIDAL PRODUCTS ARE NOT RECOMMENDED AS THEY MAY CAUSE DAMAGE TO THE CENTRIFUGE. REFRAIN FROM USING TO PREVENT VOIDING THE WARRANTY.


- Fully/partially halogenated hydrocarbons, ketones, esters, ethers, benzyls, ethyl benzenes, and all other chemicals not prescribed by the manufacturer shall not be used as they may cause damage to the rotor chamber, rotor, tube holders, accessories and centrifuge exterior and void the warranty.

TROUBLESHOOTING

NOTE: The latch must be turned completely clockwise to its stop position for the centrifuge to operate.

<p>The centrifuge does not run</p>	<ul style="list-style-type: none"> ○ Verify that the centrifuge is powered. One of the LED lights should be on. ○ Make sure the lid latch is turned completely clockwise to its stop position. ○ If the centrifuge still does not run, contact Customer Service.
<p>The rotor does not spin freely</p>	<ul style="list-style-type: none"> ○ Make sure nothing has fallen into the rotor chamber, following the procedure above. ○ If nothing obstructs the rotor, the rotor may be damaged. Contact Customer Service for further assistance.
<p>The centrifuge makes a rattling noise when running</p>	<ul style="list-style-type: none"> ○ Stop the centrifuge. Open the lid. ○ Wearing PPE, remove tubes and tube holders/buckets and look for fallen objects or debris. Carefully reach inside the rotor chamber with a tool to remove them. ○ Inspect the rotor, tube holders or buckets for damage. ○ If the tube holders or buckets have any damage, even slight, safely dispose of them and replace them. ○ If the rotor appears damaged, contact Customer Service for further assistance.
<p>Excessive noise or vibration when the centrifuge is running</p>	<ul style="list-style-type: none"> ○ Verify that all four centrifuge feet are properly seated on a flat surface. ○ Ensure that the load is balanced according to instructions in the “Balancing Loads” section of this manual. ○ Make sure that nothing has fallen into the rotor chamber.
<p>The centrifuge stops and beeps continuously</p>	<p>The load is not balanced. Press the UNLOCK button, open the lid, and balance the load as recommended elsewhere in this manual.</p>
<p>The cycle time and speed are not set to the desired value</p>	<p>Check the setting by following the instructions in the section on Changing Cycle Settings. If the preset is not the desired length, follow the procedure on the same page to change the run preset time.</p>

<p>The centrifuge does not unlock after a run is completed</p>	<ul style="list-style-type: none"> ○ Wait until the rotor has come to a complete stop. If the lid knob still cannot be rotated, press the UNLOCK button and try again. <ul style="list-style-type: none"> ○ If no LED light is on, the unit is not powered and the lid will not unlock by conventional means. Remove the latch label and use a pen to manually disengage the locking mechanism. Pull the mechanism towards the control panel and then unlatch and open the lid. ○ If the unit is damaged, contact your authorized dealer or Drucker Diagnostics.
<p>The lid does not open</p>	<ul style="list-style-type: none"> ○ Ensure that the lid knob is turned fully counterclockwise. ○ If the knob cannot be turned counterclockwise, turn it fully clockwise, press UNLOCK, and turn counterclockwise. ○ If the lid remains locked after this and will not unlock, the electronics may have been damaged. Contact customer service for assistance.
<p>Clicking noise during braking gets loud</p>	<ul style="list-style-type: none"> ○ Make sure that the screw in the center of the rotor is tight.
<p>Lid does not stay up</p>	<ul style="list-style-type: none"> ○ Tighten the center screw on the lid hinge.

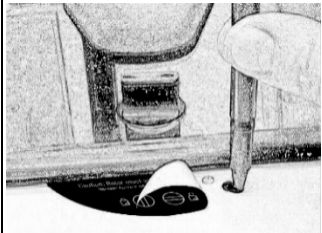

GENERAL SPECIFICATIONS

The rotor and accessories are rated for the maximum rotation frequency shown in the table below.

Apex 6	Tube Capacity	6 tubes – 3 to 10 mL
	Radius with included accessories	5 in (12.7 cm)
	Dimensions (H x W x D)	9 in x 12 in x 14 in (23 cm x 30 cm x 36 cm)
	Weight	12 lbs. (5.4 kg)
	Noise Level	61 dB
	Supply Voltage	100 – 240 (+/- 10%)
	Supply Frequency	50 - 60 Hz
	Current Consumption	2.2A at 115VAC 1.1A at 230VAC
	Centrifuge Motor	½ H.P. Brushless DC
	Maximum Speed	5,300 RPM
	Cycle Time	1 to 30 minutes (+/- 2%)
	Environmental Conditions	
	Set-up Site	Indoor Use Only
	Altitude	Up to 2,000m from Sea Level
	Ambient Temperature	5 °C to 40 °C
	Humidity	Maximum relative humidity 80% for temperatures up to 31 °C, decreasing linearly to 50% relative humidity at 40 °C
	Overvoltage Category	II
	Pollution Degree	2

Apex 12	Tube Capacity	12 tubes – 3 to 10 mL
	Radius with included accessories	5.25 in (13.3 cm)
	Dimensions (H x W x D)	9 in x 13 in x 15 in (23 cm x 33 cm x 38 cm)
	Weight	30 lbs. (13.6 kg)
	Noise Level	61 dB
	Supply Voltage	100 – 240 (+/- 10%)
	Supply Frequency	50 - 60 Hz
	Current Consumption	3.6A at 115VAC 1.8A at 230VAC
	Centrifuge Motor	½ H.P. Brushless DC
	Maximum Speed	5,200 RPM
	Cycle Time	1 to 30 minutes (+/- 2%)
	Environmental Conditions	
	Set-up Site	Indoor Use Only
	Altitude	Up to 2,000m from Sea Level
	Ambient Temperature	5 °C to 40 °C
	Humidity	Maximum relative humidity 80% for temperatures up to 31 °C, decreasing linearly to 50% relative humidity at 40 °C
	Overvoltage Category	II
Pollution Degree	2	

Apex 24	Tube Capacity	24 tubes – 3 to 10 mL
	Radius with included accessories	6 in (15.3 cm)
	Dimensions (H x W x D)	9 in x 15 in x 17 in (23 cm x 38 cm x 43 cm)
	Weight	31 lbs. (14 kg)
	Noise Level	64 dB
	Supply Voltage	100 – 200 (+/- 10%)
	Supply Frequency	50 - 60 Hz
	Current Consumption	3.6A at 115VAC 1.8A at 230VAC
	Centrifuge Motor	½ H.P. Brushless DC
	Maximum Speed	4,300 RPM
	Cycle Time	1 to 30 minutes (+/- 2%)
	Environmental Conditions	
	Set-up Site	Indoor Use Only
	Altitude	Up to 2,000m from Sea Level
	Ambient Temperature	5 °C to 40 °C
	Humidity	Maximum relative humidity 80% for temperatures up to 31 °C, decreasing linearly to 50% relative humidity at 40 °C
	Overvoltage Category	II
Pollution Degree	2	

Use only with approved accessories from the original manufacturer. A complete list of accessories is available at www.DruckerDiagnostics.com.

CALCULATING THE G-FORCE

The I.F.U.s of tube manufacturers recommend cycles at a minimum G-Force. For included accessories, a conversion table is shown below.

For other tube holders, the G-Force can be calculated if you know the RPM and the radius:

In Centimeters:

$$\text{RCF or G-force} = 0.0001118 \times \text{Rotor Radius (cm)} \times (\text{RPM})^2$$

In Inches:

$$\text{RCF or G-force} = 0.0000284 \times \text{Rotor Radius (in)} \times (\text{RPM})^2$$

	APEX 6	APEX 12	APEX 24
	Radius	Radius	Radius
	5.0 in	5.25 in	6.0 in
	12.7 cm	13.3 cm	15.3 com
RPM	G-Force	G-Force	G-Force
1000	140	150	170
1100	170	180	210
1200	200	210	250
1300	240	250	290
1400	280	290	330
1500	320	340	380
1600	360	380	450
1700	400	450	500
1800	450	500	550
1900	500	550	600
2000	600	600	700
2100	650	650	750
2200	700	700	800
2300	750	800	900
2400	800	850	1000
2500	900	900	1050
2600	950	1000	1150
2700	1050	1100	1250
2800	1100	1200	1350
2900	1200	1250	1400
3000	1300	1350	1500
3100	1350	1400	1650
3200	1450	1500	1750

	APEX 6	APEX 12	APEX 24
	Radius	Radius	Radius
	5.0 in	5.25 in	6.0 in
	12.7 cm	13.3 cm	15.3 com
RPM	G-Force	G-Force	G-Force
3300	1550	1600	1850
3400	1650	1700	2000
3500	1750	1800	2100
3600	1850	1950	2200
3700	1950	2050	2300
3800	2050	2150	2450
3900	2150	2300	2600
4000	2300	2400	2850
4100	2400	2500	2900
4200	2500	2600	3000
4300	2600	2750	3150
4400	2750	2900	N/A
4500	2900	3000	N/A
4600	3000	3150	N/A
4700	3150	3300	N/A
4800	3300	3450	N/A
4900	3400	3600	N/A
5000	3550	3750	N/A
5100	3700	3900	N/A
5200	3850	4000	N/A
5300	4000	N/A	N/A

REPLACEMENT PARTS

DASH APEX 6

Part No.	Description
7724037K	Foot, rubber (Pack of 4)
02-001-0-0011	Rotor Assembly, Dash Apex 6
02-005-1-0010	Motor Assembly
02-006-0-0011	PC Board
7760006	Power cord
03-1-0005-0192	Internal Power Supply
02-002-1-0027	Lid Assembly
7724071K	Hinge, friction (Pack of 2)
02-002-1-0056	Seal, lid gasket
03-0-0003-0313	Open/Close Label
03-1-0007-0046K	75/100mm Tube Holder, Black (Pack of 6)
02-002-1-0120K	Kit, Dash Apex 6 Lid Tray Assy, Green LED PCBA
00-100-100-009	6 Series Soft Button Replacement Kit

DASH APEX 12

Part No.	Description
7724177K	Foot, rubber (Pack of 4)
02-006-1-0044	Locking Lid Tray Assembly, 11"
02-001-0-0009	12-Place Rotor, Horizontal
02-005-1-0012	Motor Assembly
02-006-0-0034	PC Board
7760006	Power cord
03-1-0005-0193	Power Supply
02-002-1-0041	Lid Assembly
7724071K	Hinge, friction (Pack of 2)
02-002-1-0057	Seal, lid gasket
03-0-0003-0313	Open/Close Label
03-1-0007-0046K	75/100mm Tube Holder, Black (Pack of 6)
02-006-1-0067K	Kit, D/H 12/24 Green LED PCBA Replacement
00-100-100-010	12/24 Series Soft Button & Spacer Replacement Kit
00-100-100-005	Replacement Grommet & Bushing Kit

DASH APEX 24

Part No.	Description
7728052K	Foot, rubber (Pack of 4)
02-006-1-0044	Locking Lid Tray Assembly, 11"
02-001-0-0008	24-Place Rotor, Horizontal
02-005-1-0012	Motor Assembly
02-006-0-0034	PC Board
7760006	Power cord
03-1-0005-0193	Power Supply
02-002-1-0037	Lid Assembly
7724071K	Hinge, friction (Pack of 2)
02-002-1-0058	Seal, lid gasket
03-0-0003-0313	Open/Close Label
02-004-0-0012K	4 Place Carrier, Carbon Fiber (Pack of 6)
02-006-1-0067K	Kit, D/H 12/24 Green LED PCBA Replacements
00-100-100-010	12/24 Series-Soft Button & Spacer Replacement Kit
00-100-100-005	Replacement Grommet & Bushing Kit

PREVIOUS MANUAL REVISIONS

To access previous manuals, please click the relevant link below:

[Revision G](#)

[Revision H](#)

[Revision I](#)

This operator's manual is part number 03-0-0002-0120 Rev. J

Product Family: DASH Apex Series (Apex 6, Apex 12, Apex 24)

Complies with UL61010-1/CSA C22.2 No. 61010-1 and IEC61010-2-020

Protected by U.S. Patents #6,811,531, #D718,463, & #D734,489. Other Patents Pending

FDA LISTED



INSTRUCTIONS FOR DISPOSAL OF WEEE BY USERS IN THE EUROPEAN UNION



This product must not be disposed of with other waste. Instead, it is the user's responsibility to dispose of their waste equipment by handing it over to a designated collection point for the recycling of waste electrical and electronic equipment. The separate collection and recycling of your waste equipment at the time of disposal will help to conserve natural resources and ensure that it is recycled in a manner that protects human health and the environment. For more information about where you can drop off your waste equipment for recycling, please contact your local city office, waste disposal service, or where you purchased the product.

Designed, built, and supported in the USA



200 SHADY LANE, SUITE 170 – PHILIPSBURG, PA 16866, USA

+1-866-265-1486 (U.S. ONLY) - +1-814-692-7661

CUSTOMERSERVICE@DRUCKERDIAGNOSTICS.COM

DRUCKERDIAGNOSTICS.COM

